

Fig. 1

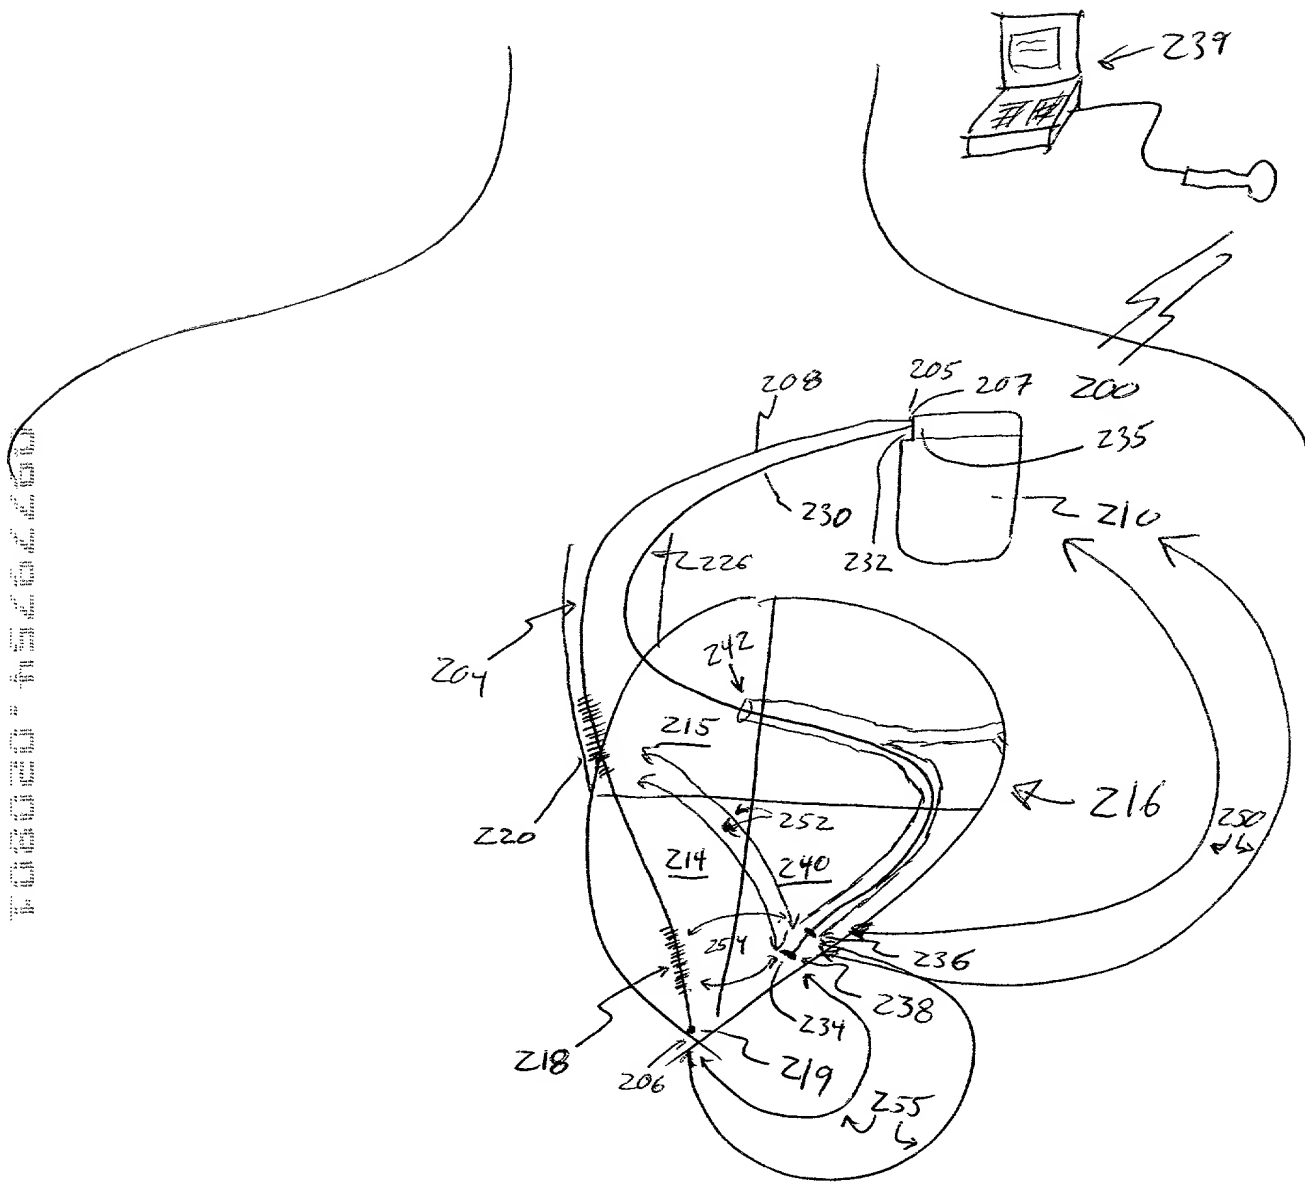


Fig. 2

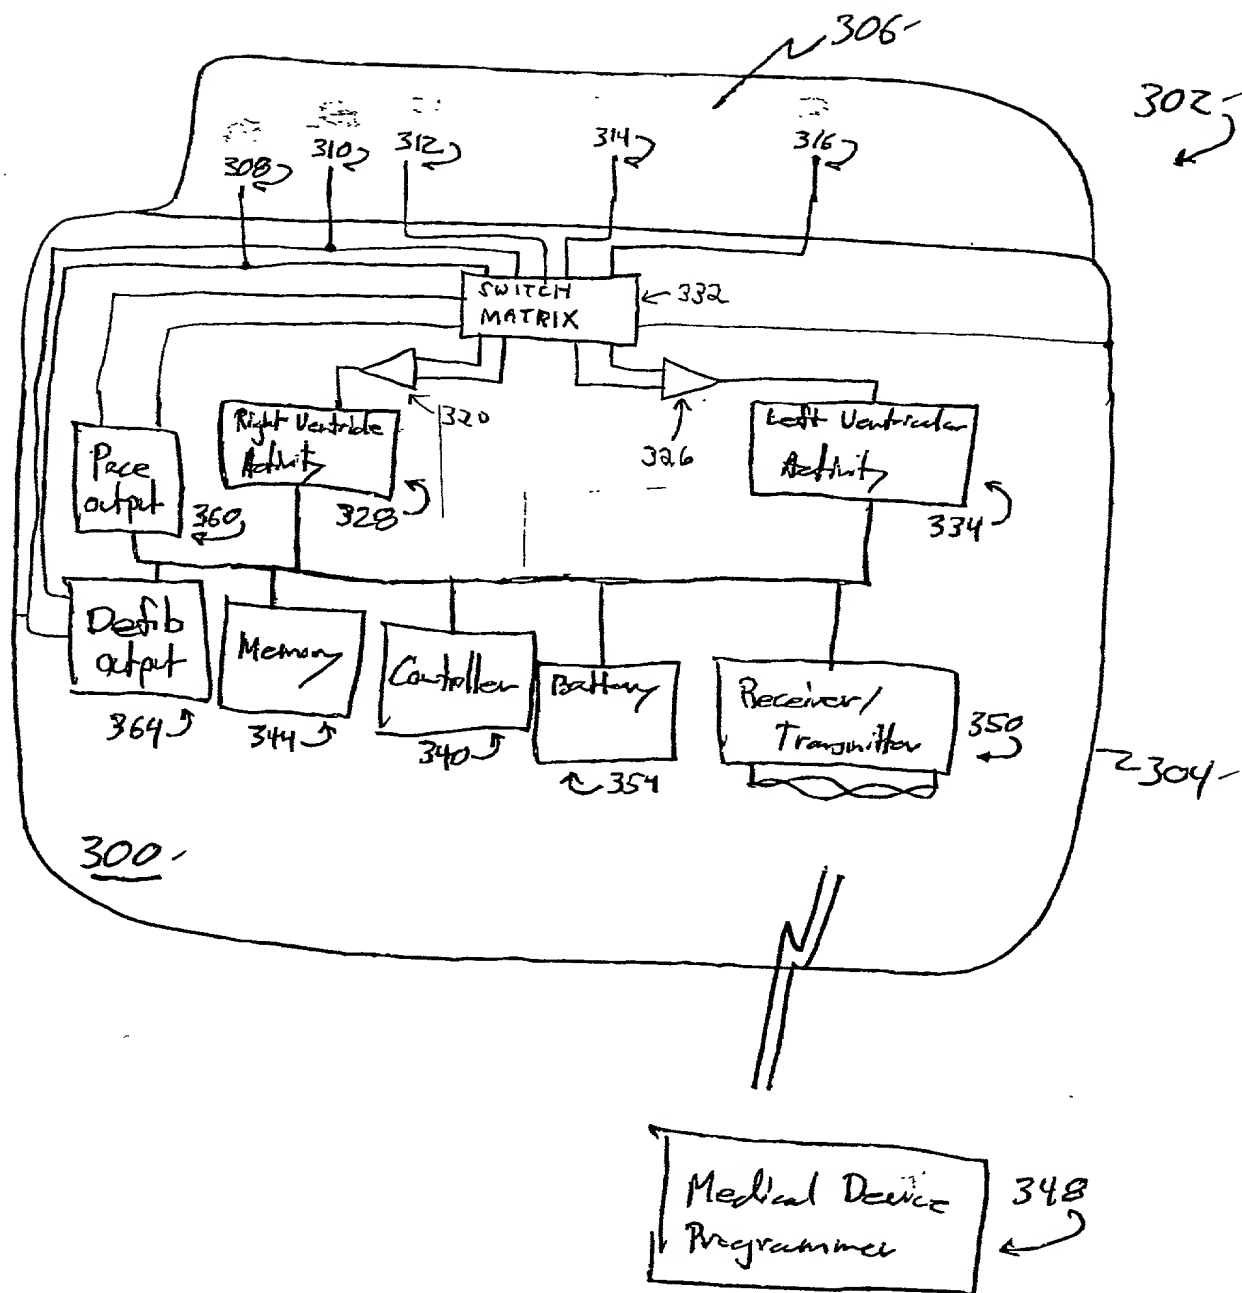


Fig. 3

Hand-drawn schematic diagram of a medical device 400, showing a catheter 404 with a distal tip 420 and a proximal handle 408. The device is shown in a curved position, with a cross-section 220 and a longitudinal section 218. The device is labeled with various reference numerals: 204, 404, 418, 420, 220, 218, 219, 430, 408, 412, and 416.

Fig. 4

00000492260

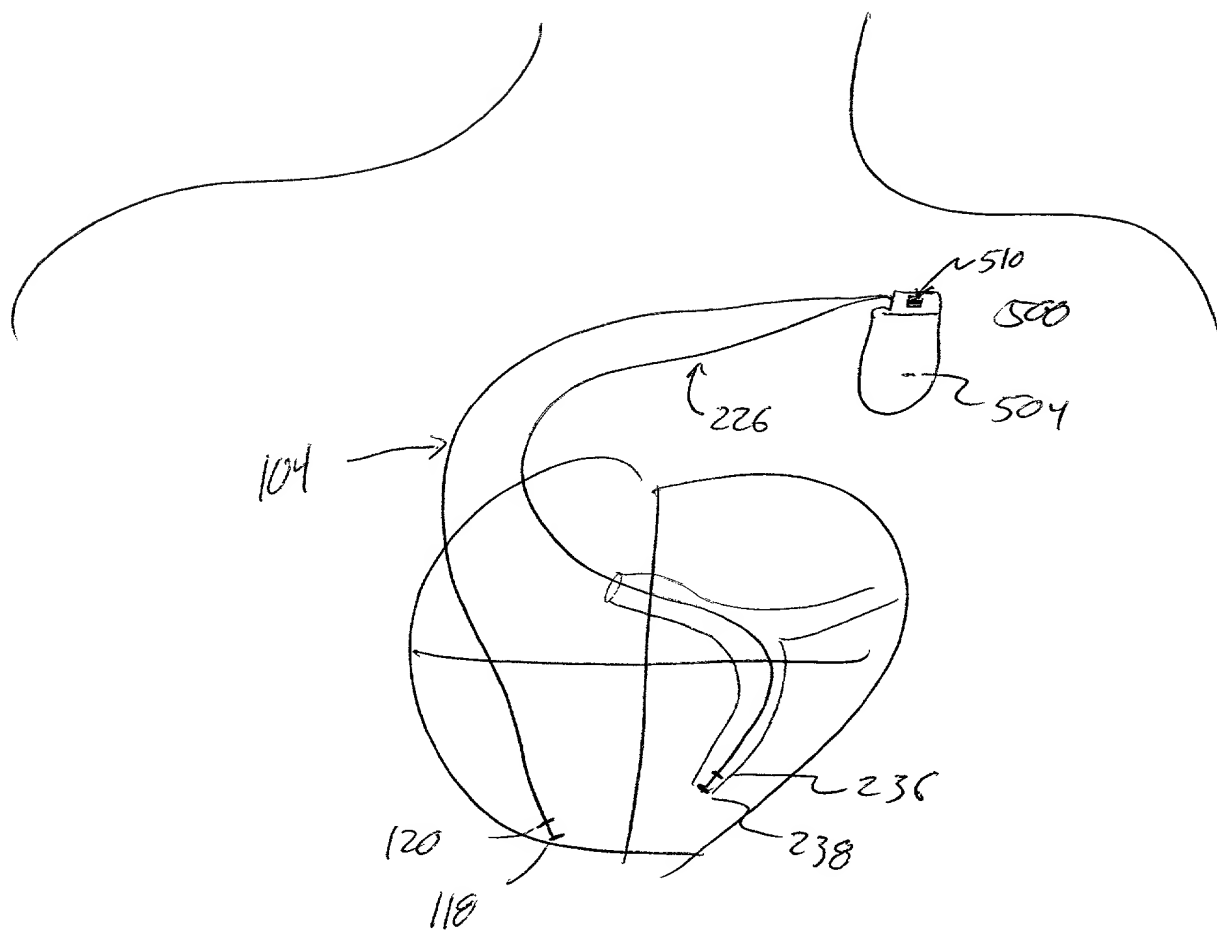


Fig 5

FIG. 6

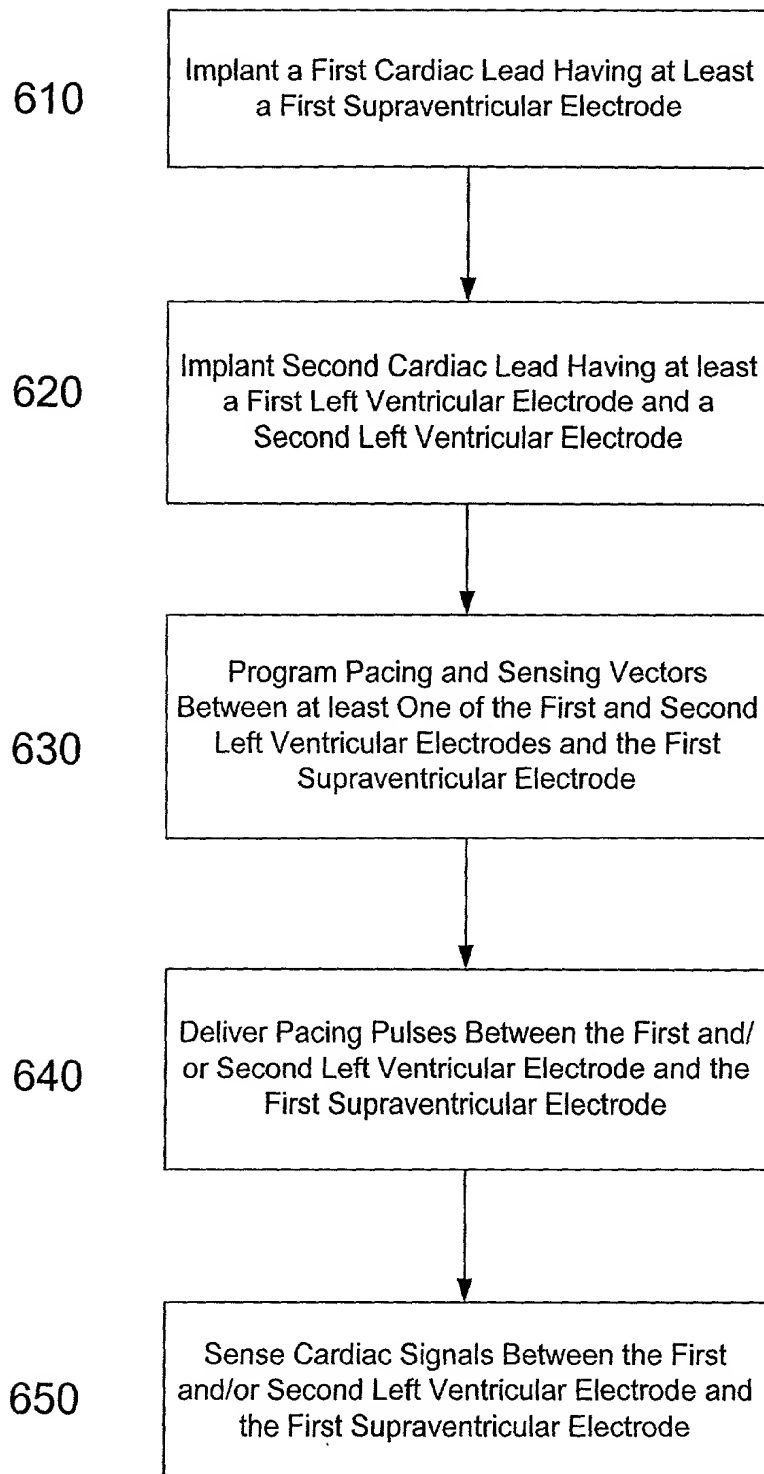


FIG. 6

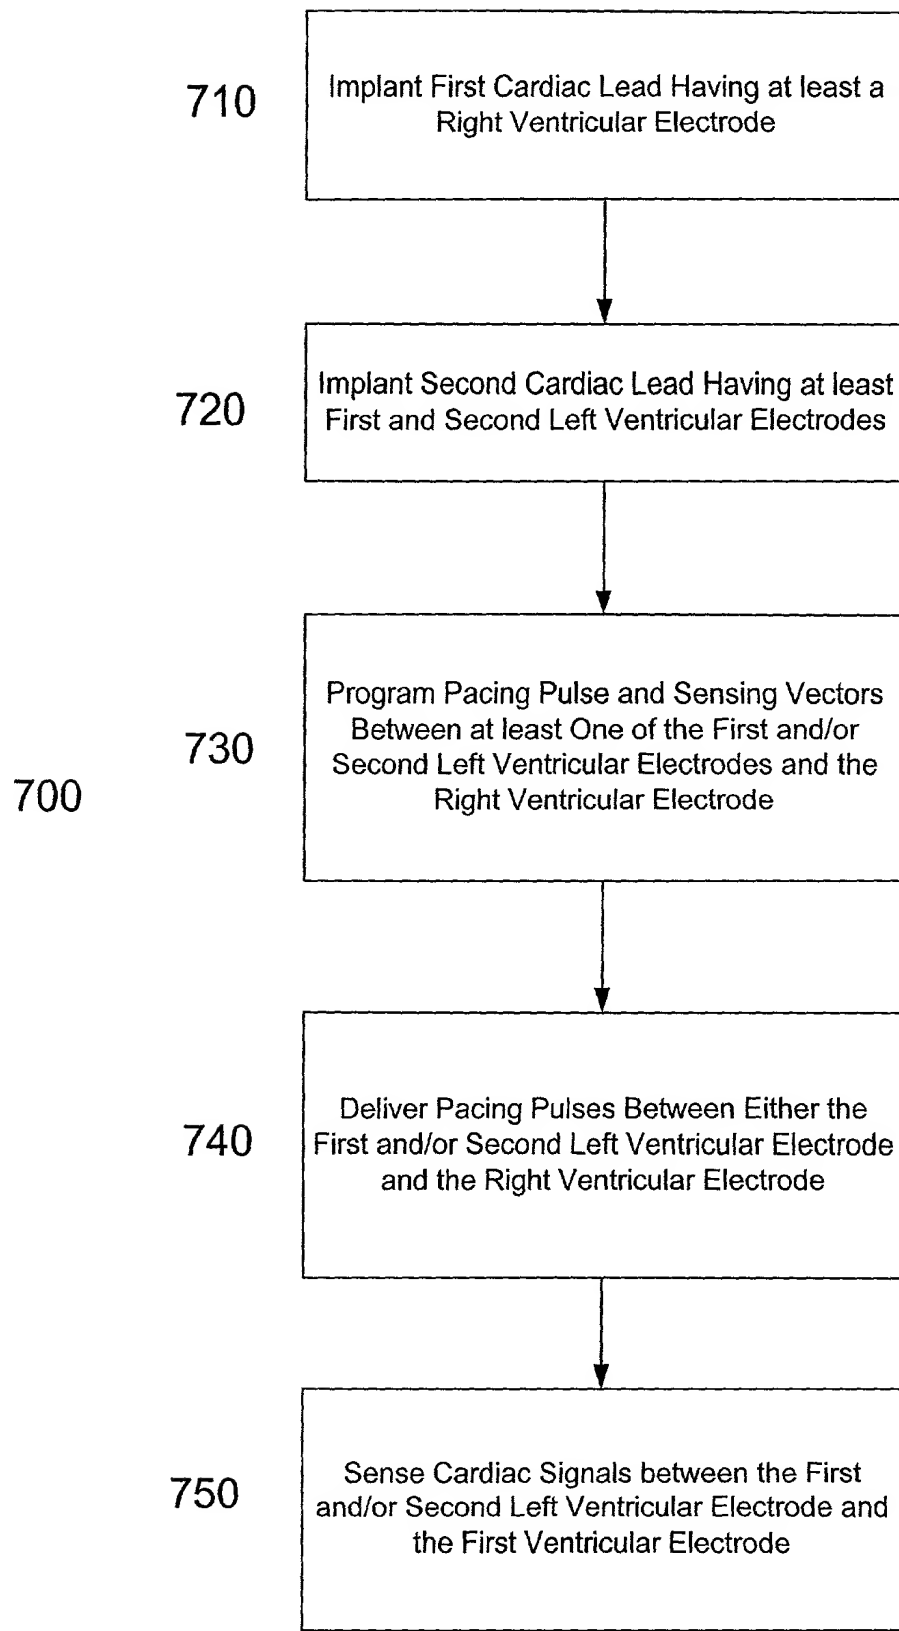


FIG. 7

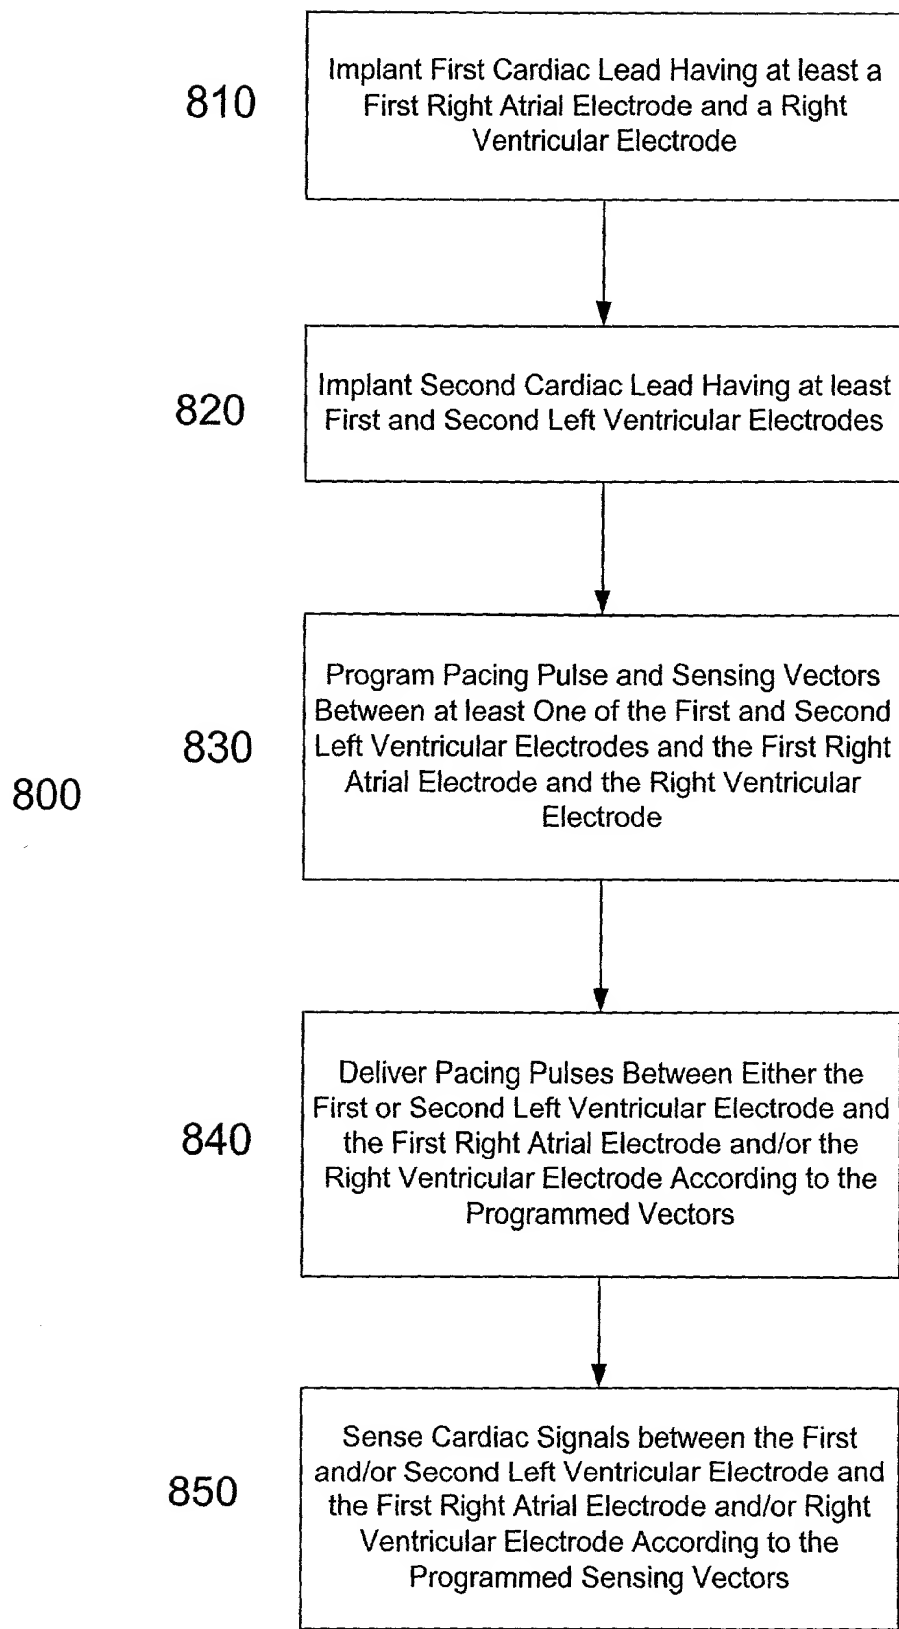


FIG. 8

900

910

Implant First Cardiac Lead Having at Least a
First Ventricular Defibrillation Electrode and a
First ventricular Pacing/Sensing Electrode



920

Delivering a Pacing Level Pulse from the First
Ventricular Defibrillation Electrode as a
Cathode to a First ventricular Pacing/Sensing
Electrode as an Anode

FIG. 9

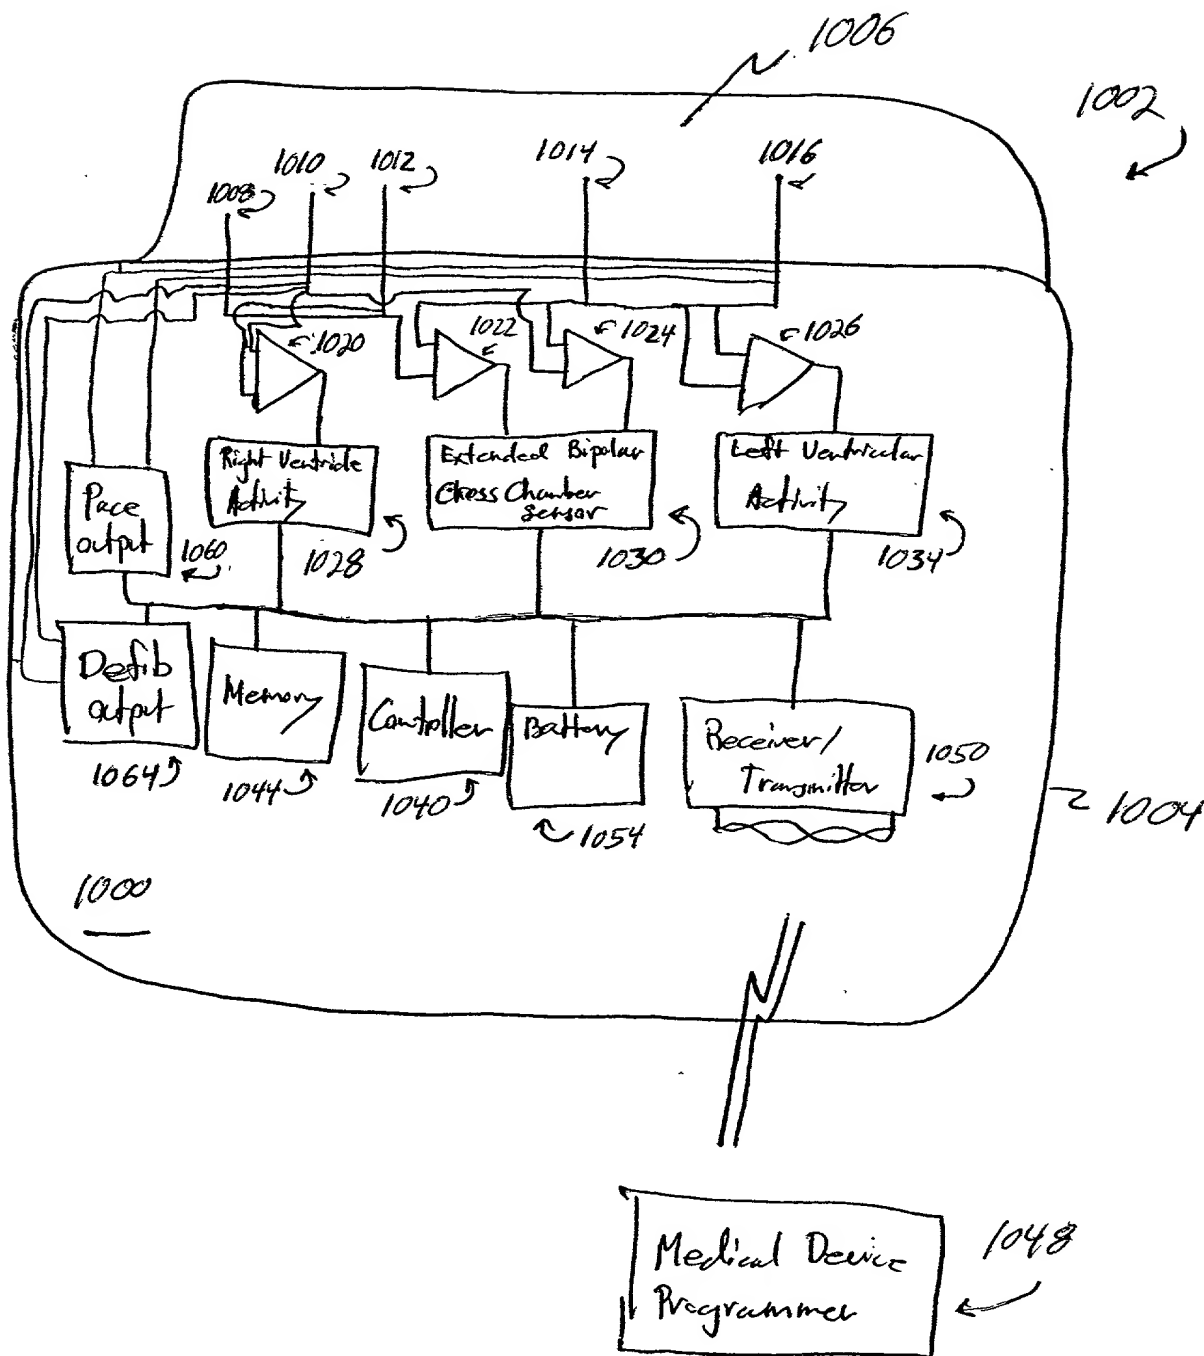


Fig. 10